


700-27-6

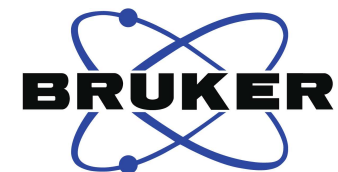

7.354  
7.351  
7.347  
7.265


1.763

Current Data Parameters  
NAME 06-05-2023  
EXPNO 14  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20230607  
Time 13.47  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 2  
SWH 8223.685 Hz  
FIDRES 0.125483 Hz  
AQ 3.9846387 sec  
RG 198.33  
DW 60.800 usec  
DE 6.50 usec  
TE 298.3 K  
D1 1.0000000 sec

===== CHANNEL f1 =====  
NUC1 1H  
P1 13.40 usec  
PLW1 16.0000000 W  
SFO1 400.1324710 MHz

F2 - Processing parameters  
SI 65536  
SF 400.1300082 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

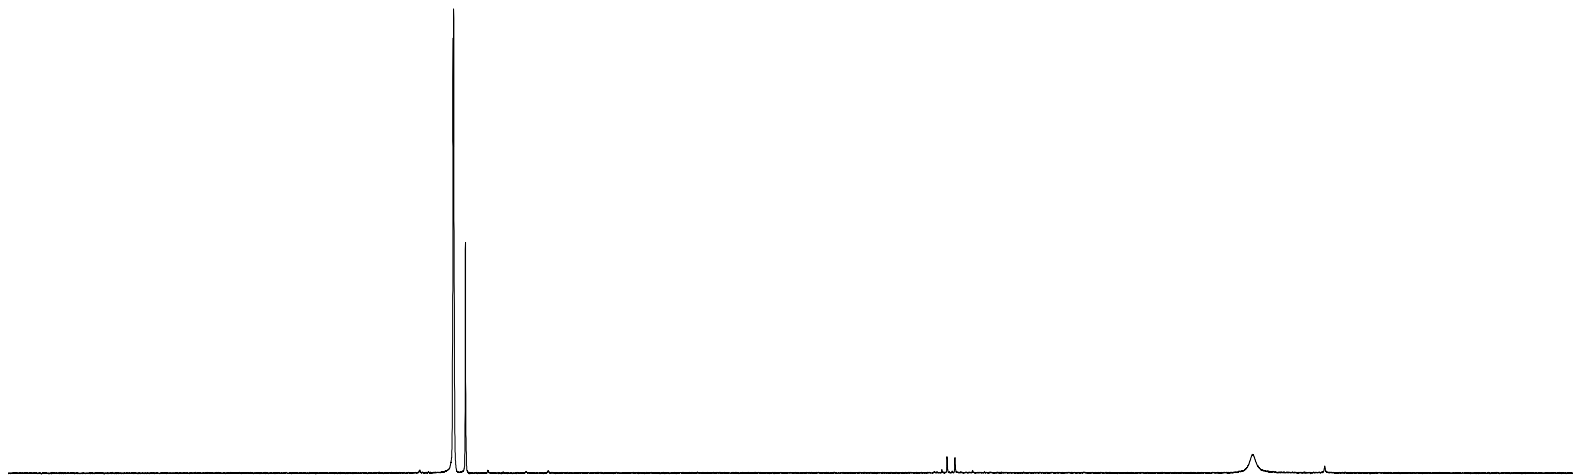

10 9 8 7 6 5 4 3 2 1 ppm

1.00