


460-32-2

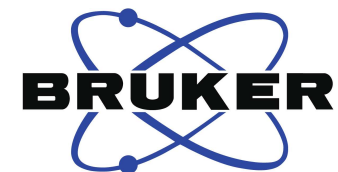

Current Data Parameters
NAME 08-26-2022
EXPNO 5
PROCNO 1


F2 - Acquisition Parameters
Date_ 20220826
Time 12.39
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 14
DS 2
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9846387 sec
RG 152.51
DW 60.800 usec
DE 6.50 usec
TE 298.1 K
D1 1.00000000 sec

===== CHANNEL f1 =====
NUC1 1H
P1 13.40 usec
PLW1 16.00000000 W
SFO1 400.1324710 MHz

F2 - Processing parameters
SI 65536
SF 400.1300082 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

— 7.265

3.470
3.451
3.431
2.759
2.734
2.714
2.709
2.695
2.689
2.677
2.670
2.665
2.645
1.539

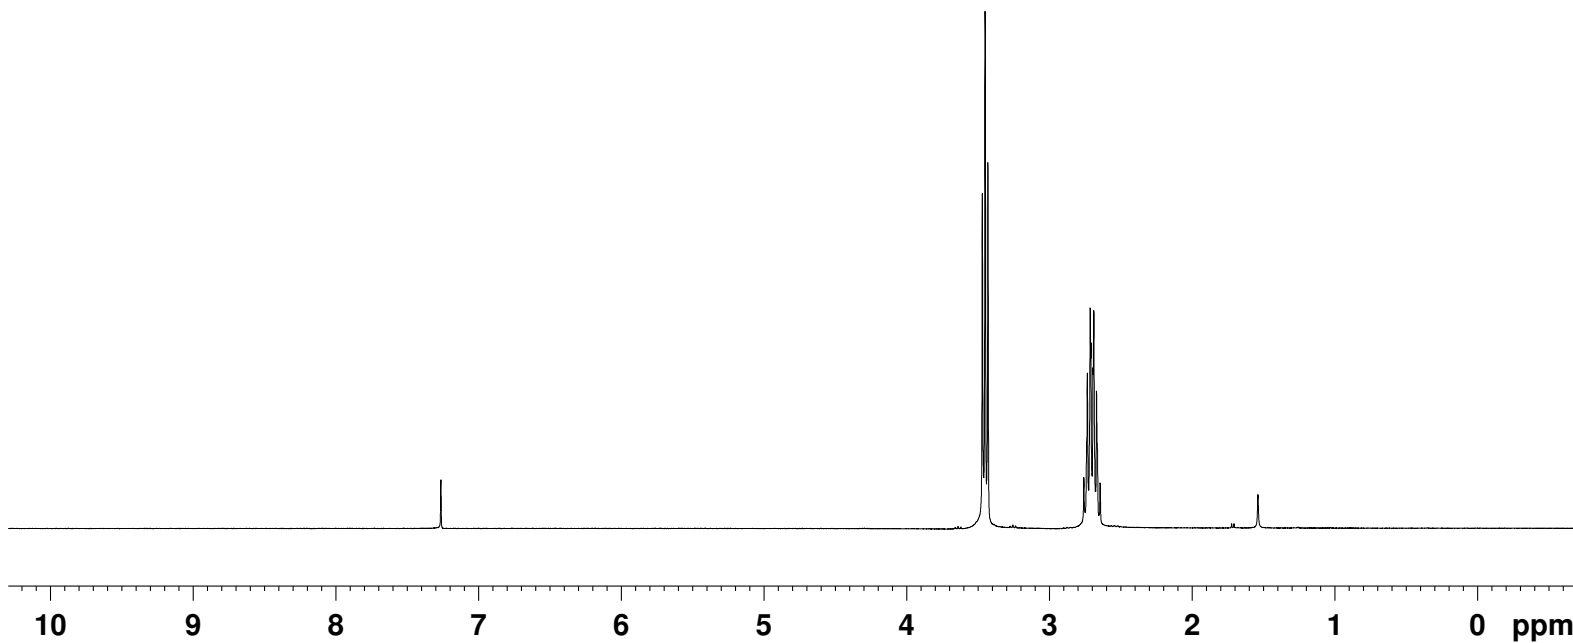

2.00
2.02