


392-41-6



--83.649
--83.703
--83.743
--83.797
--95.152
--95.205
--95.455
--95.508

--183.805
--183.899
--184.108
--184.203

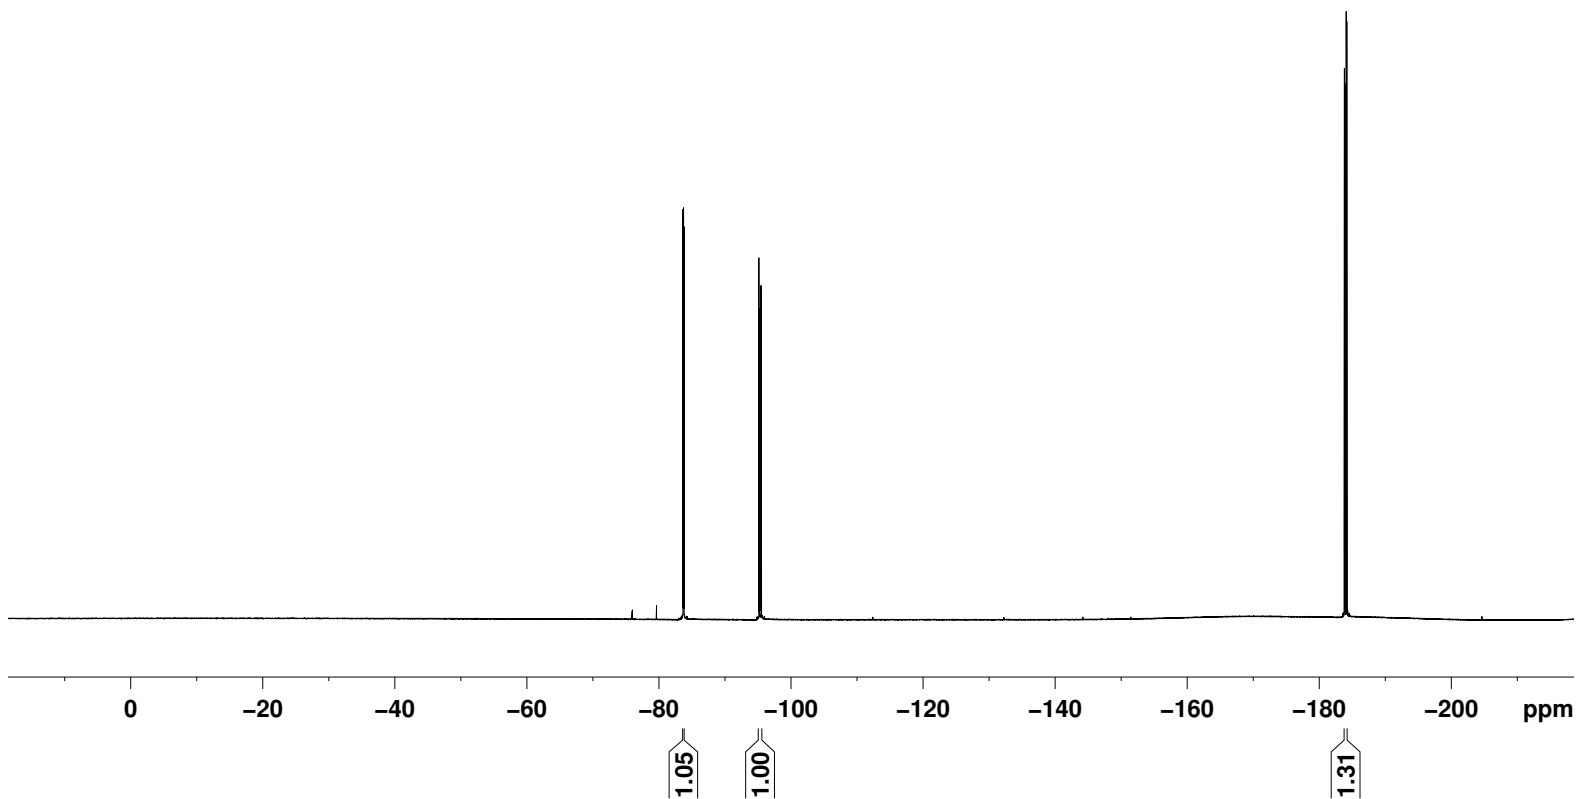

Current Data Parameters
NAME 06-21-2023
EXPNO 67
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230720
Time 13.58
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zgfhigqn.2
TD 131072
SOLVENT CDCl3
NS 16
DS 4
SWH 89285.711 Hz
FIDRES 0.681196 Hz
AQ 0.7340532 sec
RG 198.33
DW 5.600 usec
DE 6.50 usec
TE 297.9 K
D1 1.00000000 sec
D11 0.03000000 sec
D12 0.00002000 sec

=====
CHANNEL f1
NUC1 19F
P1 13.40 usec
PLW1 26.00000000 W
SFO1 376.4607164 MHz

=====
CHANNEL f2
CPDPRG2 waltz16
NUC2 1H
PCPD2 90.00 usec
PLW2 16.00000000 W
PLW12 0.35468999 W
SFO2 400.1316005 MHz

F2 - Processing parameters
SI 65536
SF 376.4983660 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00