


4089-58-1

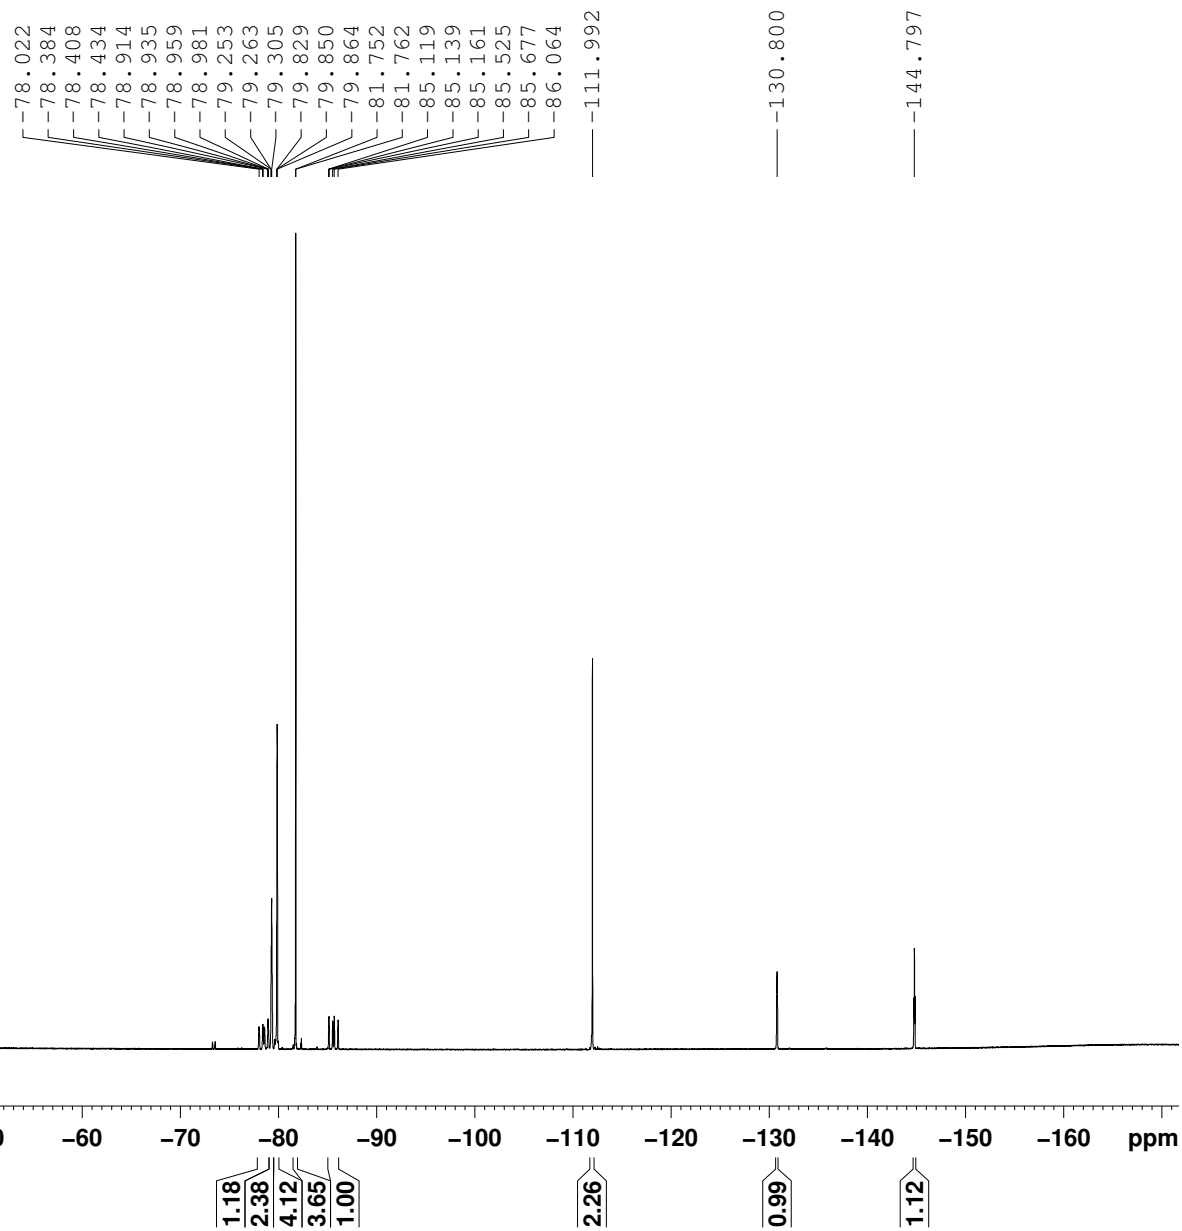

Current Data Parameters  
NAME 08-26-2022  
EXPNO 7  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220826  
Time 12.48  
INSTRUM spect  
PROBHD 5 mm PABBO BB-  
PULPROG zgfhigqn.2  
TD 131072  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 89285.711 Hz  
FIDRES 0.681196 Hz  
AQ 0.7340532 sec  
RG 198.33  
DW 5.600 usec  
DE 6.50 usec  
TE 298.2 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
D12 0.00002000 sec

==== CHANNEL f1 =====  
NUC1 19F  
P1 13.40 usec  
PLW1 26.00000000 W  
SFO1 376.4607164 MHz

==== CHANNEL f2 =====  
CPDPRG2 waltz16  
NUC2 1H  
PCPD2 90.00 usec  
PLW2 16.00000000 W  
PLW12 0.35468999 W  
SFO2 400.1316005 MHz

F2 - Processing parameters  
SI 65536  
SF 376.4983660 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00