

307-98-2




7.265
6.549
6.506
6.221
6.194
6.177
6.151
6.001
5.975
4.708
4.674
4.640
1.607

Current Data Parameters
NAME 07-29-2022
EXPNO 18
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220802
Time 12.09
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9846387 sec
RG 198.33
DW 60.800 usec
DE 6.50 usec
TE 299.5 K
D1 1.00000000 sec

===== CHANNEL f1 =====
NUC1 1H
P1 13.40 usec
PLW1 16.00000000 W
SFO1 400.1324710 MHz

F2 - Processing parameters
SI 65536
SF 400.1300077 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

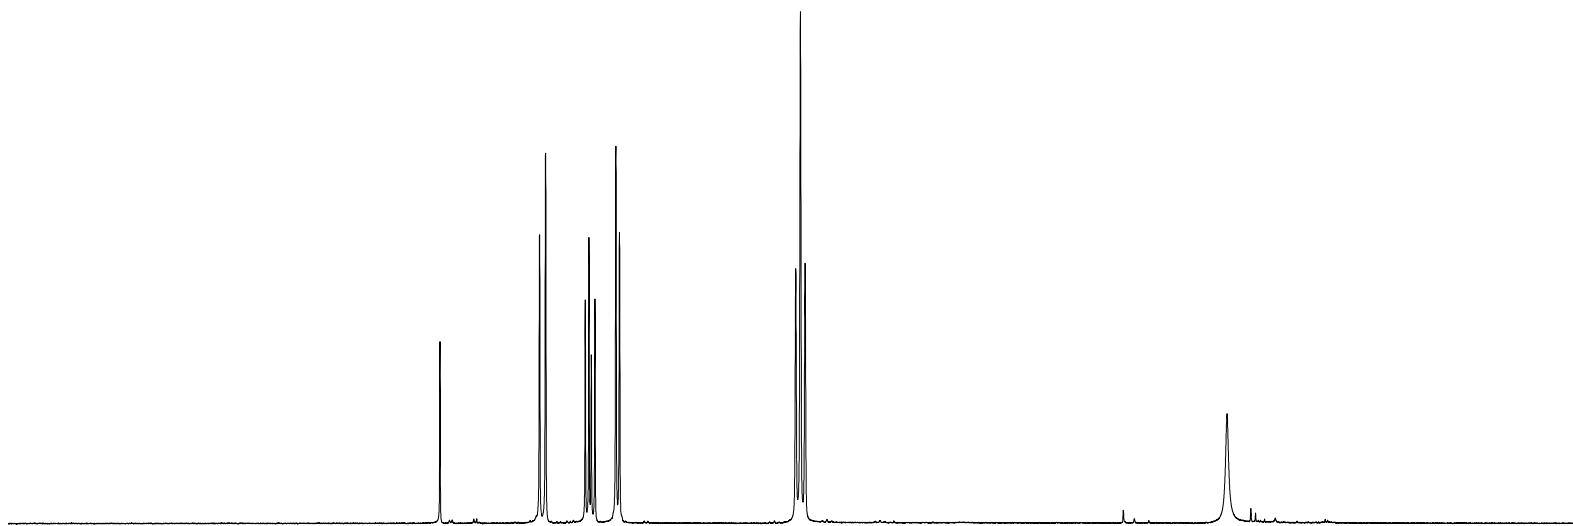

10 9 8 7 6 5 4 3 2 1 0 ppm

1.04
1.00
1.05
2.06